





KID'S FACE MASK

3-PLY EARLOOP



GENERAL INFORMATION

MANUFACTURER

Name: STL Teknoloji Ltd. Şti.

Add: Catalcesme Mah. Resadiye Cad. 186 Sok. No: 1 8
Alemdag, Cekmeköy, İstanbul/TURKEY

Authorized Representative: Mediroc Tech LTD.

CONFORMITY ASSESSMENT PROCEDURE

According to Regulation (EU) 2017/745 Article 52, the manufacturer follows the conformity assessment procedure relating to the EU declaration of conformity referred to in Article 19 after drawing up the technical documentation set out in Annexes II and III.

NOTIFIED BODY

No involvement of a Notified Body is needed for this Non-Sterile class I device.

PRODUCT INFORMATION

INTENDED USE

- Low-risk clinical applications that do not involve blood-borne pathogens or bodily fluids
- Enhancing infection control
- Preventing the risk of cross-contamination

DESCRIPTION

Rectangular face masks with a shapeable nose piece and two earloops present, one on each side, in order to hold mask in place.

Trade Mark: **Mediroc**

Model: **STL3PLYKIDS**

This product is **Type II** mask according to European Standard EU: BS EN 14683:2019

MATERIAL

Outside Layer: **Spunbond Polypropylene – SBPP (White)**
Middle Layer: **Meltblown Polypropylene – MBPP (White)**
Inner Layer: **Spunbond Polypropylene – SBPP (White)**
Nose piece: **Plastic covered iron**
Elastic Band: **Polyester**
Not formulated with Natural Rubber Latex (Latex Free)
Not formulated with DEHP
Fiberglass Free Product

MASK DIMENSIONS

Length: **175mm** Width **95mm**
Length of ear loop: **170mm**
Length of nose piece: **90mm**

MANUFACTURING

This mask is made in Turkey.



REGULATION & TESTING INFORMATION

REGULATORY INFORMATION

Product CE marked as per 93/42/EEC Directive on Medical Devices.

Class 1 Medical Device - Type II - Non-Sterile

TEST METHODS

Bacterial Filtration Efficiency (BFE)

When tested in accordance with Annex B of EN 14683, the BFE of the medical face mask shall conform to the minimum value given for the relevant type in Table 1 of EN 14683.

Breathability

When tested in accordance with Annex C of EN 14683, the differential pressure of the medical face mask shall conform to the value given in relevant type in Table 1 of EN 14683.

Microbial cleanliness (Bioburden)

The bioburden of the medical face mask shall be ≤ 30 cfu/g tested. The number of masks that shall be tested is minimum 5 of the same batch/lot.

The number of masks that shall be tested is minimum 5 of the same batch/lot.

Differential Pressure


The differential pressure of the medical face mask shall be ≤ 40 cfu/g tested. The number of masks that shall be tested is minimum 5 of the same batch/lot.

TEST	TYPE I	TYPE II	TYPE IIR
Bacterial Filtration Efficiency(BFE), (%)	≥ 95	≥ 98	≥ 98
Differential Pressure (Pa/cm ²)	<40	<40	<60
Splash Resistance Pressure (kPa)	Not Required	Not Required	$\geq 16,0$
Microbial Cleanliness (cfu/g)	≤ 30	≤ 30	≤ 30

Table – Performance Requirements for Medical Face Masks

STERILIZATION

This mask is non-sterile

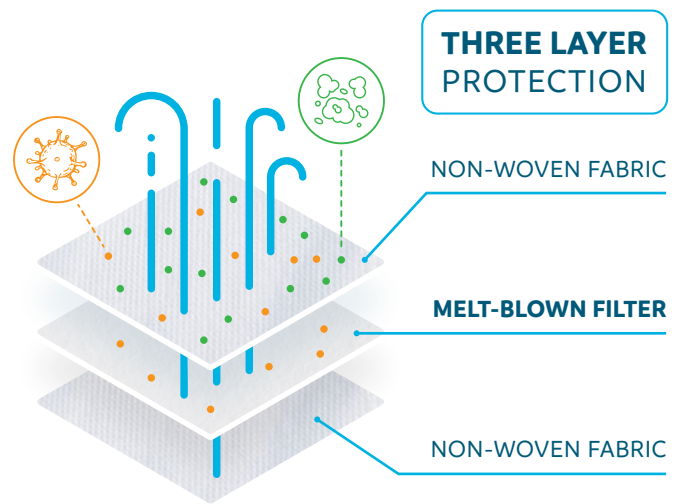

STORAGE

Store in a dry and cool place, away from intense sources of heat. Keep the masks as much as practicably possible in their dispenser box. Keep dispenser boxes as much as practicably possible in their shipper box.

PACKING

Shipping case of 1800 units

10 Units are placed within 1 box and 180 boxes are placed within 1 shipping case

Box demision: 210x105x24,5mm

Box material: 350gr Paper

Shipping case demision: 640x325x500mm

Shipping case material: Carton

SHELF LIFE

The shelf-life is 3 years after production.

The uninterrupted use duration of the device is usually less than 8 hours.

BARCODE



VISUALS






Disposable Medical
KID'S FACE MASK

DISPOSABLE MEDICAL **FACE MASK**

3-PLY EARLOOP



THREE LAYER PROTECTION

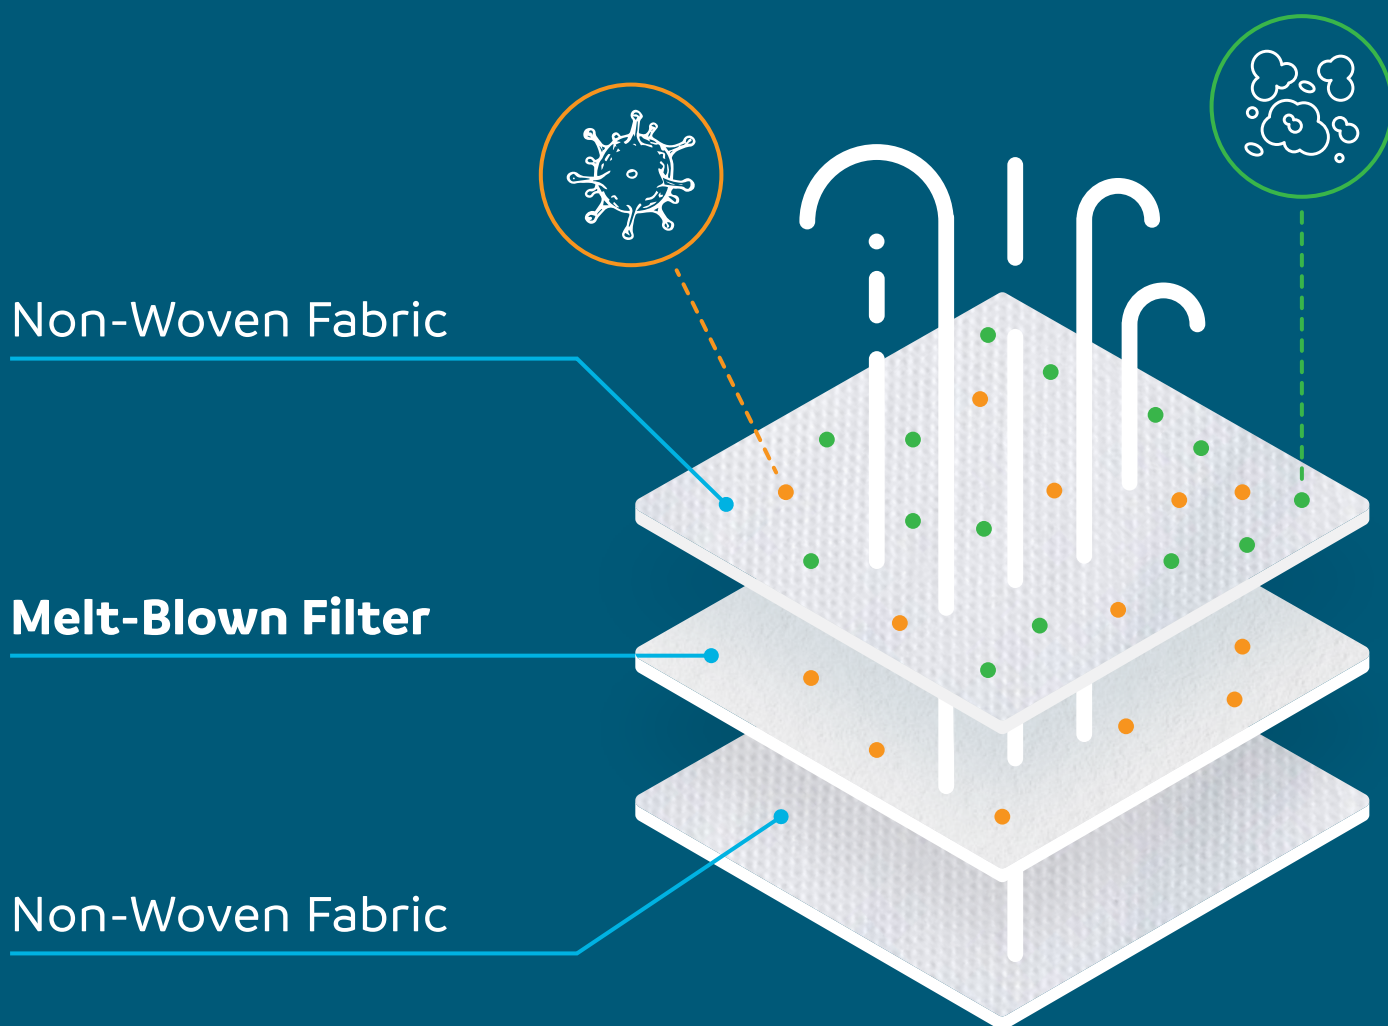



TEST REPORT

Class 1 Medical Device

Standard EU: BS EN 14683:2019

ANALYSIS REPORT

Report No. : **2011194E-R1** Report Date : 02/06/2020

Applicant : STL TEKNOLOJİ LTD. ŞTİ.
Address : Alemdağ, Çatalmeşe Mah. Reşadiye Cad, 186. Sk. No:18
Çekmeköy/ İstanbul/ Turkey

Sample : Disposable Medical Face Mask

Sample Package : Carton box
Sample Amount : 100 adet
Sampling Point : -
Sampling Date : -
Sample Lot No. : -

Sample Carrying Conditions / Preservation Technique : -

Production Date : 05/2020
Packing Date : -
Expire Date : 2023
Producer Company : STL Teknoloji Ltd. Şti.
Sample Receiving Time : 21/05/2020 10:30:00
Analysis Beginning Time : 21/05/2020 10:45:00
Analysis Completion Time : 29/05/2020

Following analysis results were obtained from the specimen which was delivered by cargo to Çevre Laboratory;

Parameters	Unit	Finding	Tip I	Tip II	Tip IIR	LR Source	Method	Information
Differential Pressure								
DP - 1	Pa/cm ²	16,73	< 40	< 40	< 60	97	EN 14683 - Annex C 122, 123, 126	
DP - 2	Pa/cm ²	19,02	< 40	< 40	< 60	97	EN 14683 - Annex C 122, 123, 126	
DP - 3	Pa/cm ²	16,52	< 40	< 40	< 60	97	EN 14683 - Annex C 122, 123, 126	
DP - 4	Pa/cm ²	17,1	< 40	< 40	< 60	97	EN 14683 - Annex C 122, 123, 126	
DP - 5	Pa/cm ²	15,92	< 40	< 40	< 60	97	EN 14683 - Annex C 122, 123, 126	
Bacterial Filtration Efficiency								
BFE - 1	%	99,6	≥95	≥98	≥98	97	EN 14683 - Annex B 122, 124, 129	
BFE - 2	%	99,6	≥95	≥98	≥98	97	EN 14683 - Annex B 122, 124, 129	
BFE - 3	%	99,6	≥95	≥98	≥98	97	EN 14683 - Annex B 122, 124, 129	
BFE - 4	%	99,9	≥95	≥98	≥98	97	EN 14683 - Annex B 122, 124, 129	



Merve BİRAH
Assistant Laboratory Responsible of
Microbiology Laboratory



Approved by
02/06/2020
Ömer Yasin BALIK
Laboratory Manager

ANALYSIS REPORT

Report No. : 2011194E-R1

Report Date : 02/06/2020

Following analysis results were obtained from the specimen which was delivered by cargo to Çevre Laboratory;

Parameters	Unit	Finding	Tip I	Tip II	Tip IIR	LR Source	Method	Information
BFE - 5	%	99,6	≥95	≥98	≥98	97	EN 14683 - Annex B	122, 124, 129
Mean Positive Control Count	cfu	2395	-	-	-	-	EN 14683 - Annex B	
Negative Control Count	cfu	<1	-	-	-	-	EN 14683 - Annex B	
Mean Particle Size (MPS)	µm	2,9	-	-	-	-	EN 14683 - Annex B	
Microbial Limit - Bioburden								
Bioburden - 1	cfu/g	22	≤30	≤30	≤30	97	ISO 11737-1	120, 131
Bioburden - 2	cfu/g	16	≤30	≤30	≤30	97	ISO 11737-1	120, 131
Bioburden - 3	cfu/g	19	≤30	≤30	≤30	97	ISO 11737-1	120, 131
Bioburden - 4	cfu/g	16	≤30	≤30	≤30	97	ISO 11737-1	120, 131
Bioburden - 5	cfu/g	22	≤30	≤30	≤30	97	ISO 11737-1	120, 131

Source of Limit Ranges : 97 Medikal Yüz Maskelerinin Test Metodları ve Performans Gerekksinimleri (EN 14683)

A: Acceptable NA: Not Acceptable

MU: Measurement Uncertainty

Method	EN : European Standard ISO : International Organization for Standardization
Information	120 : Bioburden : Aerobic Bacteria and Mold-Yeast Pozitive Controls : Bacillus atrophaeus Extract Fluid : Peptone, Tween with Sodium Chloride Extract Fluid Volume : 300 mL Plating Method : Membrane Filtration Agar Medium : Tryptic Soy Agar for Aerobic Bacteria Count and Sabouraud Dextrose Agar with Chloramphenicol for Mold and Yeast Count Recovery Efficiency : Repetitive Rinse Method Aerobic Bacteria : Plates are incubated 3 days at 30-35°C, then enumerated. Yeast - Mould : Plates are incubated 5-7 days at 20-25°C, then enumerated. 122 : Conditioning Parameters : 85± 5 relative humidity and 21± 5 °C de minimum 4 hours 123 : Flow rate during testing : 8 L/dk 124 : Flow rate during testing : 28.3 L/dk 126 : The mask analyzed according to the results of Differential Pressure provides EN 14683 Table 1. Type I, Type II and Type IIR limits. 129 : The mask analyzed according to the results of Bacterial Filtration Efficiency (BFE) provides EN 14683 Table 1. Type I, Type II and Type IIR limits. 131 : The mask analyzed according to the results of Microbial Limit - Bioburden provides the EN 14683 Table 1. Type I, Type II and Type IIR limits.

R1 : This report supersedes 29/05/2020 date 2011194E number of report which is invalid.



Merve BİRAH
 Assistant Laboratory Responsible of
 Microbiology Laboratory



Approved by
 02/06/2020
Ömer Yasin BALIK
 Laboratory Manager

ANALYSIS REPORT

Report No. : 2011194E-R1

Report Date : 02/06/2020

Note

1. When request, the conformit assessment is carried out in accordance with the legal regulations and standards or the decision rules which are agreed with the customer.
2. Descriptive information about the samples / sampling in the analysis report has been declared by the customer. Our laboratory is not responsible for the legal losses.
3. Analysis report covers samples/sampling that comes to the laboratory.
4. This report and results don't not be copied and printed partially or completely without permission of Cevre Industrial Analysis Laboratory for any commercial and advertising purposes.
5. This report shall not be used official purposes related to Enviromental Regulations.
6. The test report without sign is not valid.

End of Report



Merve BİRAH
Assistant Laboratory Responsible of
Microbiology Laboratory



Approved by
02/06/2020
Ömer Yasin BALIK
Laboratory Manager



EU DECLARATION OF CONFORMITY & CERTIFICATION

EU DECLARATION OF CONFORMITY



Mediroc Disposable Medical Face Mask

Name and address of manufacturer : STL TEKNOLOJİ LTD. ŞTİ.
Alemdağ, Çatalçeşme Mah. Reşadiye Cad. 186. Sok. No:18
Çekmeköy/İstanbul/Turkey

Product Name : Disposable Medical Face Mask

Brand Name :  mediroc

Product Types : Type II, Non-Sterile

Authorized Representative : Mediroc Tech Ltd.

This declaration confirms that the product meets the essential requirements of following directive(s) and standart(s). The conformity was based on;

Applied Directive(s) : Medical Devices Directive 93/42/EEC as amended according to the Directive 2007/47/EC

Applied Standard(s) : EN 14683:2019 Medical Face Masks - Requiremenst and test methods

International Standards : ISO 13485:2016 / ISO 9001:2015(QMS)

The declaration has been carried out in accordance with individual rules and conditions. Evaluation has been carried out in accordance with:

Test Report(s) No : 20011194E-R1

Test Conducted by : Cevre Industrial Analysis Laboratory

Test Lab. Adress : Merkez Mahallesi Tatlıpınar Sokak No: 13 Mart Plaza Kat: 2/A
Kağıthane/İstanbul

Issue Date : 02/06/2020

Revision Date/No : -

* The undersigned herewith declarer that the above-mentioned product(s) meet the provisions of the following EC Council Directives and harmonized standards, All supporting documentations are retained under the premises of the manufacturer.

İstanbul/Turkey
05.06.2020

General Manager

STL TEKNOLOJİ LTD. ŞTİ.
Çatalmeşe Mah. Reşadiye Cad. 186 Sk. No: 18
Alemdağ - Çekmeköy - İstanbul - TÜRKİYE
Sarıgazi V.D.: 773 030 161 Te. Sic. No: 575043
Mersis No: 0773030161000010
<http://benceiyi.com> - info@benceiyi.com
Tel.: 02163145521 Fax: 02163145523



SYNDICATE OF INTERNATIONAL SYSTEM CERTIFICATIONS

This Certificate has been awarded to

STL TEKNOLOJİ LİMİTED ŞİRKETİ

ÇATALMEŞE MAH. REŞADİYE CAD. 186. SOK. NO:18
ÇEKMEKÖY / İSTANBUL / TÜRKİYE

In recognition of the organization's Managements System which complies with

EN 14683:2019+AC:2019

The scope of activities covered by this certificate is defined below

MANUFACTURE, SALES AND EXPORTS OF TEXTILE PRODUCTS, MEDICAL PROTECTIVE CLOTHING, MASK, PROTECTIVE OVERALLS, BONNET, GLOVES, OVERSHOE, APRON, SURGERY APRON FOR PATIENTS AND DOCTOR, STRETCHER COVER, DEAD BODY BAG, COLONOSCOPY SHORTS, PATIENT SHORTS, DISINFECTANT LIQUIDS, ANTIBACTERIAL SOAP AND LIQUIDS, SURFACE AND SKIN CLEANING MATERIALS, FACE PROTECTOR VISORS, SUITCASE

TEKSTİL ÜRÜNLERİ, MEDİKAL KORUYUCU KIYAFET, MASKE, KORUYUCU TULUM, BONE, ELDİVEN, GALOŞ, ÖNLÜK, HASTA VE DOKTOR İÇİN AMELİYAT ÖNLÜĞÜ, SEDYE ÖRTÜSÜ, CESET TORBAS, KOLONOSKOPİ ŞORTU, HASTA ŞORTU, DEZENKFEKTAN SIVILAR, ANTİBAKTERİYAL SABUN VE SIVILAR, YÜZEY VE CİLT TEMİZLİK MALZEMELERİ, YÜZ KORUYUCU SİPERLİK, VALİZ ÜRETİMİ, SATIŞI VE İHRACATI

Certificate Number: **SISTURAC052020104**

Date of Issue of Original Certificate: **06.05.2020**

Date of Issue of latest certificate: **27.05.2020**

Expiry Date: **05.05.2021**

SYNDICATE OF INTERNATIONAL SYSTEM CERTIFICATIONS

Managing Director



Note: This certificate is valid only if produced with the continuation letter after the surveillance is carried out successfully.

The Organization's documentation and Implementation has been reviewed and found to comply with the relevant standard rules. This certificate of Registration is based on the evaluation of the mentioned scope given above. Organization is responsible for maintaining the responsibilities of the relevant standard rules. Any significant changes in the scope of the certification or standard referred above render this certificate invalid.

Corporate office(SIS):- Plot No. 1539, 2nd Floor, Sector-4,Gurgaon-122001, Haryana, India.
International office(SIS):- URB. Santa Ana Cal. German, Scherieber 276, San Isidro, Lima, Peru 15047.
Email us :-support@siscertifications.com, info@siscertifications.co.in. Call:- +91-9654721646
Web:- <http://www.siscertifications.co.in>, www.siscertifications.com
The status of this certificate can be verified on "<http://www.siscertifications.co.in>".

Issue No.: 02

CERTIFICATE OF COMPLIANCE





SYNDICATE OF INTERNATIONAL SYSTEM CERTIFICATIONS

This Certificate has been awarded to

STL TEKNOLOJİ LİMİTED ŞİRKETİ

ÇATALMEŞE MAH. REŞADİYE CAD. 186. SOK. NO:18
ÇEKMEKÖY / İSTANBUL / TÜRKİYE

In recognition of the organization's Management System
which complies with

ISO 9001:2015(QMS)

The scope of activities covered by this certificate is defined below

MANUFACTURE, SALES AND EXPORTS OF TEXTILE PRODUCTS, MEDICAL PROTECTIVE CLOTHING, MASK, PROTECTIVE OVERALLS, BONNET, GLOVES, OVERSHOE, APRON, SURGERY APRON FOR PATIENTS AND DOCTOR, STRETCHER COVER, DEAD BODY BAG, COLONOSCOPY SHORTS, PATIENT SHORTS, DISINFECTANT LIQUIDS, ANTIBACTERIAL SOAP AND LIQUIDS, SURFACE AND SKIN CLEANING MATERIALS, FACE PROTECTOR VISORS, SUITCASE

TEKSTİL ÜRÜNLERİ, MEDİKAL KORUYUCU KIYAFET, MASKE, KORUYUCU TULUM, BONE, ELDİVEN, GALOŞ, ÖNLÜK, HASTA VE DOKTOR İÇİN AMELİYAT ÖNLÜĞÜ, SEDYE ÖRTÜSÜ, CESET TORBASİ, KOLONOSKOPİ ŞORTU, HASTA ŞORTU, DEZENKFEKTAN SIVILAR, ANTİBAKTERİYAL SABUN VE SIVILAR, YÜZEY VE CİLT TEMİZLİK MALZEMELERİ, YÜZ KORUYUCU SİPERLİK, VALİZ ÜRETİMİ, SATIŞI VE İHRACATI

Certificate Number: **SISTURQ0420202085**

Date of Issue of Original Certificate: **22.04.2020**

Date of Issue of latest certificate: **27.05.2020**

Expiry Date: **22.04.2021**

SYNDICATE OF INTERNATIONAL SYSTEM

Managing Director

Note: This certificate is valid only if produced with the continuation letter after the surveillance is carried out successfully.

The Organization's documentation and Implementation has been reviewed and found to comply with the relevant standard rules. This certificate of Registration is based on the evaluation of the mentioned scope given above. Organization is responsible for maintaining the responsibilities of the relevant standard rules. Any significant changes in the scope of the certification or standard referred above render this certificate invalid. This is an accredited certificate issued by SIS Certifications Pvt. Ltd. sanctioned for issue by International Accreditation Services, 3060 Saturn Street Suite 100 Brea, California 92821-1732, USA.

Corporate office(SIS):- Plot No. 1539, 2nd Floor, Sector-4, Gurgaon-122001, Haryana, India.
International office(SIS):- URB. Santa Ana Cal. German, Schrieber 276, San Isidro, Lima, Peru 15047.
Email us :-support@siscertifications.com, info@siscertifications.co.in. Call:- +91-9654721646
Web:- <http://www.siscertifications.co.in>, www.siscertifications.com
The status of this certificate can be verified on "<http://www.siscertifications.co.in>".

Issue No.: 02





SYNDICATE OF INTERNATIONAL SYSTEM CERTIFICATIONS



CE ATTESTATION OF CONFORMITY

Related Directives :

MEDICAL DEVICES 93/42/EEC-----TIBBİ CİHAZLAR DİREKTİFİ 93/42/EEC

Class Sınıf: CLASS 1 / SINIF 1, NON STERILE

Description of Product :

MEDICAL MASK

TIBBİ MASKE

Manufactured by

STL TEKNOLOJİ LİMİTED ŞİRKETİ

ÇATALMEŞE MAH. REŞADİYE CAD. 186. SOK. NO:18 ÇEKMEKÖY / İSTANBUL / TÜRKİYE

Certificate No.: SISTURCE052020705

Issue Date (Original): 06.05.2020

Issue Date(Latest): 26.05.2020


Expiry Date: 05.05.2021



SYNDICATE OF INTERNATIONAL SYSTEM CERTIFICATIONS

This Certificate is issued under the following conditions:

- 1.It applies only to the above referenced models of the medical devices.
- 2.It does not imply that the SIS has performed any surveillance or control of their manufacture.
- 3.The manufacture is obligated to assure conformity of all in medical devices of the respective model to type assessed by the mean of this certificate.
- 4.The certificate remains valid until the manufacturing condition, the quality system or relevant legislation are changed .
- 5.After fulfilling of the relevant EU legislation requirements, the manufacture shall affix to each medical device, of the above referenced models, the CE-marketing according to this example:


Managing Director



Note: This certificate is valid only if produced with the continuation letter after the surveillance is carried out successfully.

The Organization's documentation and Implementation has been reviewed and found to comply with the relevant standard rules. This certificate of Registration is based on the evaluation of the mentioned scope given above. Organization is responsible for maintaining the responsibilities of the relevant standard rules. Any significant changes in the scope of the certification or standard referred above render this certificate invalid.

Corporate office(SIS):- Plot No. 1539, 2nd Floor, Sector-4,Gurgaon-122001, Haryana, India.
International office(SIS):- URB. Santa Ana Cal. German, Scherieber 276, San Isidro, Lima, Peru 15047.
Email us :-support@siscertifications.com, info@siscertifications.co.in. Call:- +91-9654721646
Web:- <http://www.siscertifications.co.in>, www.siscertifications.com
The status of this certificate can be verified on "<http://www.siscertifications.co.in>".

Issue No.: 02

CERTIFICATE OF REGISTRATION



CERTIFICATE of Registration



*This is to Certify that the
Medical Devices – Quality Management System
of*

STL TEKNOLOJİ LİMİTED ŞİRKETİ

**ÇATALMEŞE MAH. REŞADİYE CAD. 186. SOK. NO:18 ÇEKMEKÖY /
İSTANBUL / TÜRKİYE**

**has been independently assessed and is compliant
with the requirements of**

ISO 13485:2016

This Certificate is applicable to the following product or service ranges:

**MANUFACTURE, SALES AND EXPORTS OF MEDICAL PROTECTIVE CLOTHING, MASK,
PROTECTIVE OVERALLS, BONNET, GLOVES, OVERSHOE, APRON, SURGERY APRON FOR
PATIENTS AND DOCTOR, STRETCHER COVER, DEAD BODY BAG, COLONOSCOPY SHORTS,
PATIENT SHORTS, DISINFECTANT LIQUIDS, ANTIBACTERIAL SOAP AND LIQUIDS,
SURFACE AND SKIN CLEANING MATERIALS, FACE SHIELDS
MEDİKAL KORUYUCU KIYAFET, MASKE, KORUYUCU TULUM, BONE, ELDİVEN, GALOŞ,
ÖNLÜK, HASTA VE DOKTOR İÇİN AMELİYAT ÖNLÜĞÜ, SEDYE ÖRTÜSÜ, CESET TORBASİ,
KOLONOSKOPİ ŞORTU, HASTA ŞORTU, DEZENKFEKTAN SIVILAR, ANTİBAKTERİYEL
SABUN VE SIVILAR, YÜZEY VE CİLT TEMİZLİK MALZEMELERİ, YÜZ KORUYUCU
SİPERLİK ÜRETİMİ, SATIŞI VE İHRACATI**

:: Certificate No :: TR52007H

Date of initial registration 22 April 2020

Date of this Certificate 22 May 2020

Surveillance audit on or before 21 April 2021

Recertification Due / Certificate expiry 21 April 2023

This Certificate is property of Staunchly Management & System Services Ltd. and remains valid
subject to satisfactory surveillance audits.

Director

STAUNCHLY MANAGEMENT & SYSTEM SERVICES LTD.

Suite 48, 88-90 Hatton Garden, London, EC1N 8PN.

Phone : +44 345 680 0199

Email : info@staunchlyservices.com Web : www.staunchlyservices.com

SMS/F109A/17/REV02


For precise and updated information concerning the present certificate mail to info@staunchlyservices.com

This Certificate is the property of Staunchly Management & System Services Private Limited and shall be returned immediately when demanded





PACKAGING

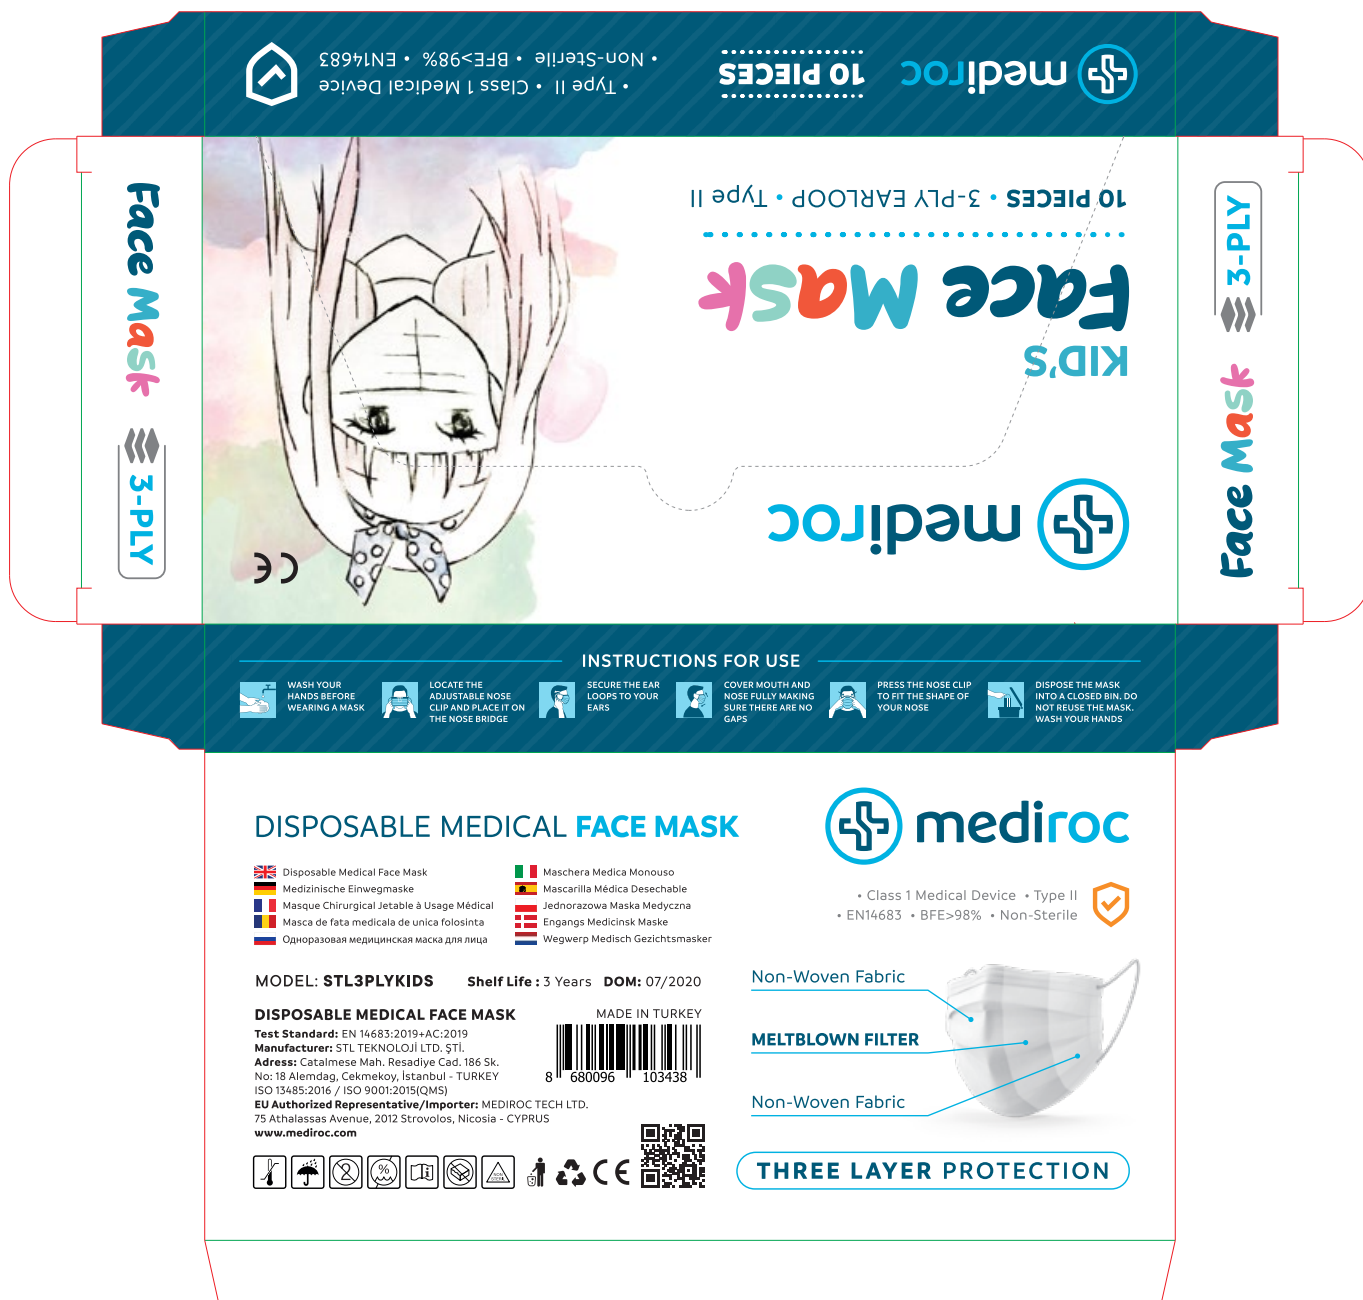

• Type II • Class 1 Medical Device
• Non-Sterile • BFE>98% • EN14683

10 PIECES • 3-PLY EARLOOP • Type II

Face Mask 3-PLY

Face Mask 3-PLY

Face Mask KID'S

mediroc

INSTRUCTIONS FOR USE



WASH YOUR HANDS BEFORE WEARING A MASK



LOCATE THE ADJUSTABLE NOSE CLIP AND PLACE IT ON THE NOSE BRIDGE



SECURE THE EAR LOOPS TO YOUR EARS



COVER MOUTH AND NOSE FULLY MAKING SURE THERE ARE NO GAPS



PRESS THE NOSE CLIP TO FIT THE SHAPE OF YOUR NOSE



DISPOSE THE MASK INTO A CLOSED BIN. DO NOT REUSE THE MASK. WASH YOUR HANDS

DISPOSABLE MEDICAL FACE MASK



Disponible Medical Face Mask
Medizinische Einwegmaske
Masque Chirurgical Jetable à Usage Médical
Mascara de fata medicala de unica folosinta
Одноразовая медицинская маска для лица

Maschera Medica Monouso
Mascarilla Médica Desechable
Jednorazowa Maska Medyczna
Engangs Medicinsk Maske
Wegwerp Medisch Gezichtsmasker

• Class 1 Medical Device • Type II
• EN14683 • BFE>98% • Non-Sterile



MODEL: STL3PLYKIDS Shelf Life : 3 Years DOM: 07/2020

DISPOSABLE MEDICAL FACE MASK

Test Standard: EN 14683:2019+AC:2019
Manufacturer: STL TEKNOLOJİ LTD. ŞTİ.
Address: Catalmes Mah. Resadiye Cad. 186 Sk.
No: 18 Alemdag, Cekmekoy, Istanbul - TURKEY
ISO 13485:2016 / ISO 9001:2015(QMS)

EU Authorized Representative/Importer: MEDIROC TECH LTD.
75 Athalassas Avenue, 2012 Strovolos, Nicosia - CYPRUS
www.mediroc.com

MADE IN TURKEY




Non-Woven Fabric

MELTBLOWN FILTER

Non-Woven Fabric

THREE LAYER PROTECTION



INSTRUCTIONS FOR USE 1) Wash your hands before wearing a mask. 2) Locate the adjustable nose clip and place it on the nose bridge. 3) Secure the ear loops to your ears. 4) Cover mouth and nose fully making sure there are no gaps. 5) Press the nose clip to fit the shape of your nose. 6) Dispose the mask into a closed bin. Do not reuse the mask. Wash your hands.

ИНСТРУКЦИИ ПО ИСПОЛЬЗОВАНИЮ 1) Вымойте руки перед тем, как надеть маску. 2) Поместите регулируемый зажим для носа на переносицу. 3) Закрепите ушные петли в удобное положение на ушах. 4) Убедитесь, что маска полностью покрывает область рта и носа. 5) Накиньте на зажим для носа так, чтобы он плотно прилегал. 6) После использования - утилизируйте маску и вымойте руки. Не используйте маску повторно.

MODE D'EMPLOI 1) Lavez-vous les mains avant de porter un masque. 2) Localisez le clip de nez réglable et placez-le sur le haut du nez. 3) Fixez les élastiques à vos oreilles. 4) Couvrez complètement la bouche et le nez en vous assurant qu'il n'y a pas d'oubli. 5) Appuyez sur le pince nez pour l'adapter à la forme de votre nez. 6) Jeter le masque dans une poubelle fermée. Ne pas réutiliser le masque. Lavez-vous les mains après.

INSTRUCCIONES DE USO 1) Lávase las manos antes de usar una máscara. 2) Ubique la pinza nasal y colóquela en el puente de la nariz. 3) Asegure el arnés a ambos lados de tus oídos. 4) Cubrase la boca y la nariz, asegurando de que no hay huecos. 5) Presione el clip de la pinza nasal para adaptarlo a la forma de su nariz. 6) Deseche la máscara en un cesto cerrado. No reutilice la máscara. Lávese las manos. **ISTRUZIONI PER L'USO** 1) Lavarsi le mani prima di indossare una maschera. 2) Individuare il nasello regolabile e posizionarlo sul ponte del naso. 3) Fissare i passanti per le orecchie. 4) Coprire completamente la bocca e il naso assicurandosi che non ci siano spazi vuoti. 5) Premere il ferma nasale per adattarlo alla forma del naso. 6) Disporre la maschera in un contenitore chiuso. Non riutilizzare la maschera. Lavarsi le mani.

INSTRUKCJA UŻYCIA 1) Umij ręce przed założeniem maski. 2) umieść zaciąg maski na nosie. 3) umocuj maskę na uszach. 4) usta i nos powinny być całkowicie zakryte. 5) użyj zaciągu na nosie, aby dopasować maskę do kształtu twojego nosa. 6) użyj maski wyrzuć do kosza. Nie używać maski ponownie. Umij ręce.

GEBRUCHSANWEISUNG 1) Waschen Sie Ihre Hände bevor Sie eine Maske anziehen. 2) Suchen Sie den verstellbaren Nasenclip und platzieren Sie ihn auf der Nasenbrücke. 3) Befestigen Sie die Maske mit den Gummibändern an Ihren Ohren. 4) Decken Sie Mund und Nase vollständig ab und stellen Sie sicher, dass kein Luftspalt vorhanden ist. 5) Passen Sie den Nasenclip der Form Ihrer Nase an. 6) Entsorgen Sie die Maske in einem geschlossenen Behälter. Verwenden Sie die Maske nicht mehrmals. Waschen Sie die Hände. **GEBRUUKSAANWIJZING** 1) Was je handen voordat je een masker draagt. 2) Localiseer de neuskleem en plaats deze streep op de neusbrug. 3) Pak masker bij de elastieken en plaats deze om de oren. 4) De onderkant van je masker spreid je nu open tot onder je kin zodat neus, mond en kin volledig zijn afgedekt en het masker goed aansluit. 5) Druk de neuskleem aan zodat het vorm van je neus aanneemt. 6) Gooi het masker in de afvalbak en raak deze niet onnodig aan. Was opnieuw je handen.

BRUGSANVISING 1) Vaski händer eller brug håndsprit før du tager ansigtsmaske på. 2) Find den justerbare næseclip og sæt den på næsen. 3) Fastgør ørestropperne til ørerne. 4) Sælg for, at munden og næsen er fuldstændig dækket af masken. 5) Tilpas næseclipsen til næsen. 6) Efter brug smides masken væk - helst i en lukket affaldsbeholder. Masken må ikke genbruges. Vask hænder efter brugen af masken.

INSTRUCȚIUNI DE FOLOSIRE 1) Spălați-vă mâinile înainte de a folosi masca. 2) Localizați clema de nas reglabilă și așezați-o pe podul nasului. 3) Fixați buclele de elastic după ureche. 4) Acoperiți gura și nasul complet. Asigurați-vă că nu există spațiu liber. 5) Apăsați clema pentru a se potrivi cu forma nasului. 6) Aruncați masca într-un Cos și închideți copul.Nu refolosiți. Spălați-vă pe mâini.



THANK YOU!

